Print on Plain White Paper (Part No. 122919)

Installation Instructions

9A156 Exam Light
Used on Model 491

Intended Use
To supply illumination to patient during examination.

Kit Components

Description	Qty
Exam Light Assembly	1
Light Mounting Bracket	1
Screws	8

Installation

(1) Remove headrest (not shown) and remove screws securing back cover (Item 1).

(2) Unplug cord from electrical PC board (Item 2). Remove board from back casting (Item 3).

(3) Align holes in bracket (Item 4) with holes in chair back. Reassemble electrical PC board on top of bracket using the (4) 10-32 x 5/8” screws supplied.

(4) Remove back upholstery (Item 5) from the chair back casting.

(5) Reposition back cover onto chair back casting. While holding back cover in position, use the installed bracket as a template to mark the location of the four holes onto the inside of the back cover from the front side of the chair back.

(6) Drill (4) 1/4” hole in the back cover centered with each of the marks. Reinstall back cover with original hardware onto back of chair back.

(7) Secure light assembly (Item 7) to back cover using (4) #8-32 x 3/4” (Item 6) screws provided.

(8) Reinstal upholstery (Item 5).

(9) Plug light into receptacle and adjust light arm to desired position. Tighten locking handle on light base.

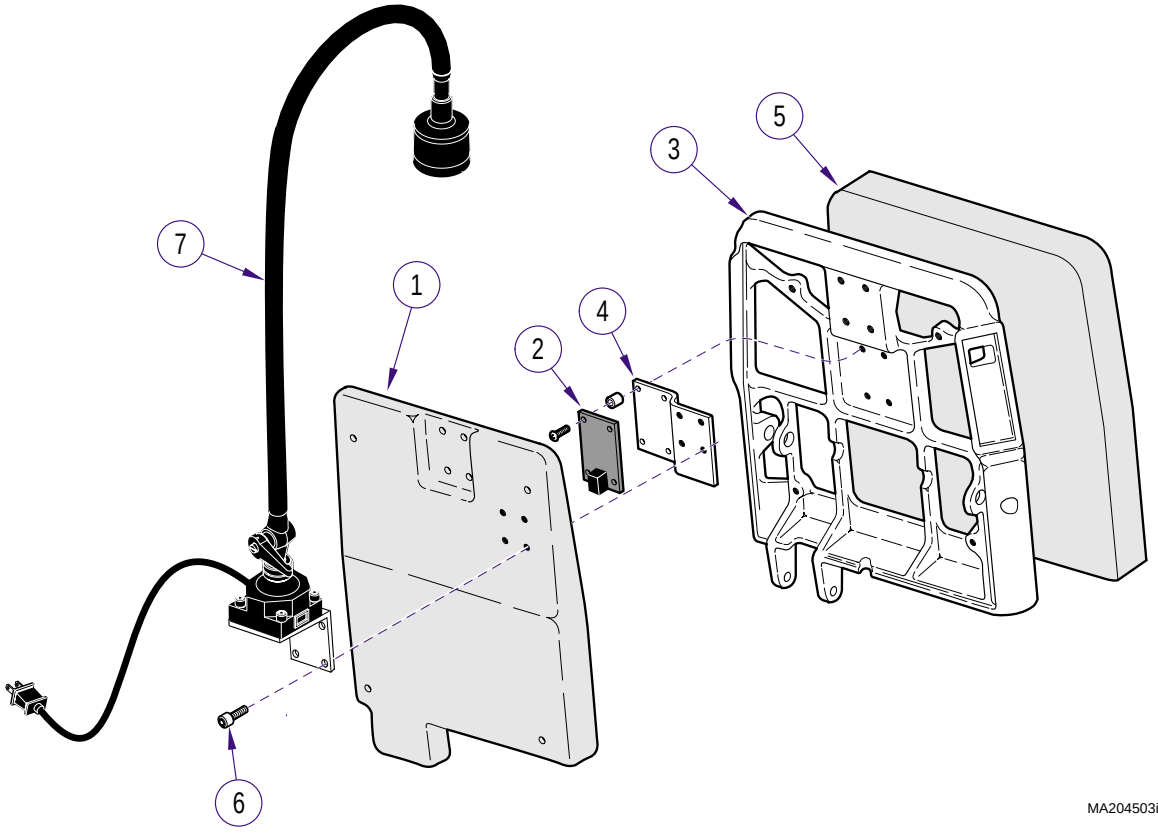

© Midmark Corporation - 2002